


**HTSD3 ASTM High temperature****1**

Sample name : BP CALIBRANT  
Acquired on : 17-May-10, 16:40:31  
Processed on : 8/3/2010 10:33:11 AM  
Sample type : Calib 25950.100  
Method name : ht750c\_p  
Operator : psw  
Sequence name : 0630A.S

Vial : 90  
Injection : 1  
Sample (g) : 0.0000  
Solvent (g) : 0.0000  
ISTD (g) : 0.0000

Data File : 0517A\090F0101.D

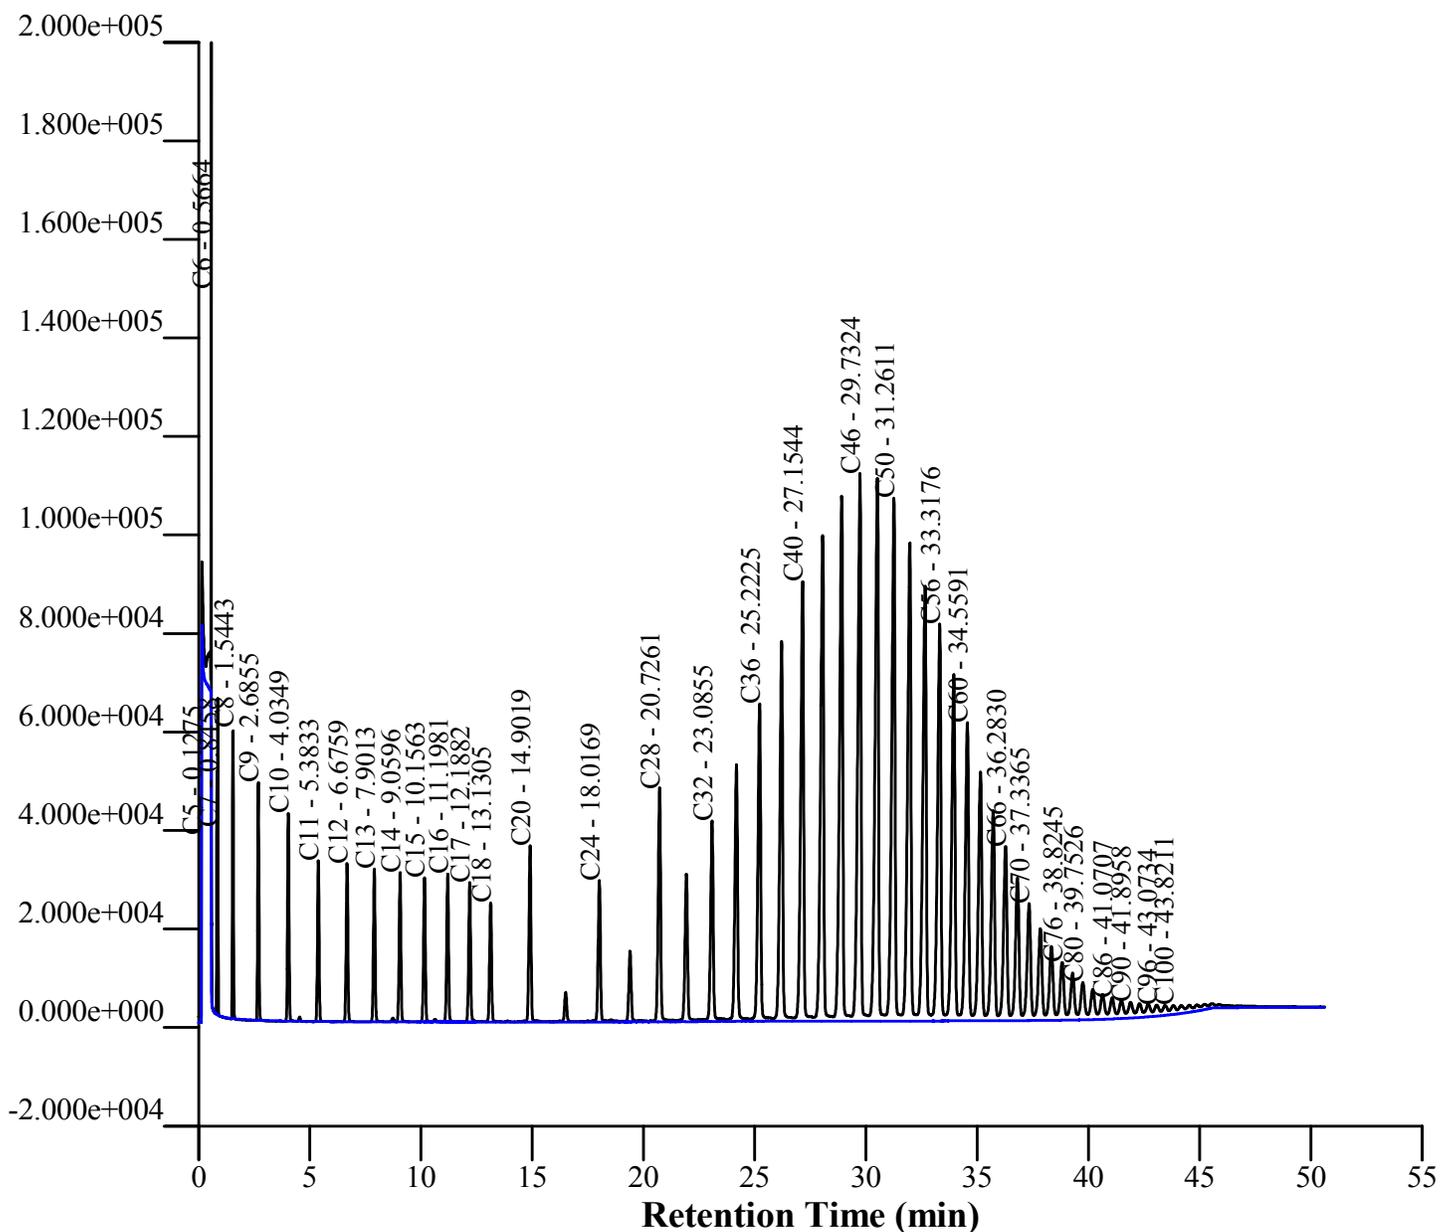

**HTSD3 ASTM High temperature****2**

Sample name : BP CALIBRANT  
 Acquired on : 17-May-10, 16:40:31  
 Processed on : 8/3/2010 10:33:11 AM  
 Data File : 0517A\090F0101.D

Vial : 90  
 Injection : 1

**Calibration report:**

Nr	Component	BP(°F)	Rt(min)	Skew	Resolution
1	C5	97	0.127		
2	C6	156	0.566		
3	C7	208	0.846		
4	C8	259	1.544		
5	C9	304	2.686		
6	C10	345	4.035		
7	C11	385	5.383		
8	C12	421	6.676		
9	C13	455	7.901		
10	C14	489	9.060		
11	C15	520	10.156		
12	C16	549	11.198		
13	C17	576	12.188		
14	C18	601	13.130		
15	C20	651	14.902	1.26	
16	C24	736	18.017		
17	C28	808	20.726		
18	C32	871	23.085		
19	C36	925	25.222		
20	C40	972	27.154	2.01	
21	C46	1033	29.732		
22	C50	1067	31.261		
23	C56	1112	33.318		
24	C60	1139	34.559	1.70	
25	C66	1175	36.283		
26	C70	1197	37.336	1.37	
27	C76	1227	38.825		
28	C80	1247	39.753	1.15	
29	C86	1276	41.071		
30	C90	1292	41.896		
31	C96	1314	43.073		
32	C100	1328	43.821		
<b>33</b>	<b>C110</b>	<b>1355</b>	<b>45.223</b>		
<b>34</b>	<b>C120</b>	<b>1382</b>	<b>46.625</b>		

## HTSD3 ASTM High temperature

3

Sample name : BP CALIBRANT  
 Acquired on : 17-May-10, 16:40:31  
 Processed on : 8/3/2010 10:33:11 AM  
 Data File : 0517A\090F0101.D

Vial : 90  
 Injection : 1

